

ENG

Product Data Sheet:

## **HUMAN sCD14 ELISA**

Catalogue number:

**RHK320-01R**

**RHK320-02R**

**For research use only!**

Example Version

1. INTENDED USE	3
2. INTRODUCTION	3
3. KIT FEATURES	3
4. TEST PRINCIPLE	4
5. TECHNICAL HINTS	5
6. REAGENT SUPPLIED	6
7. MATERIALS REQUIRED BUT NOT PROVIDED	6
8. WARNINGS AND PRECAUTIONS	7
9. PREPARATION OF REAGENTS	8
10. PREPARATION OF SAMPLES	9
11. ASSAY PROCEDURE	10
12. CALCULATIONS	11
13. QUALITY CONTROL	11
14. TROUBLESHOOTING	12
15. REFERENCES	13
16. EXPLANATION OF SYMBOLS	14

## 1. INTENDED USE

The human sCD14 ELISA kit is to be used for the *in vitro* quantitative determination of human sCD14 in serum, plasma, urine, breast milk and cell culture supernatant samples. This kit is intended for laboratory research use only and is not for use in diagnostic or therapeutic procedures.

The analysis should be performed by trained laboratory professionals.

## 2. INTRODUCTION

CD14, the 55-kDa glycoprotein known to function as a receptor for LPS, is expressed mainly on the surface of monocytes/macrophages, and polymorphonuclear cells (PMN), the cells responsible for scavenging of LPS and bacteria. Although monocytes and PMN are the main CD14 expressing cells few reports have described CD14 expression on B-cells, mesangial cells and basophils. The plasma protein LBP plays an important role in the LPS-CD14 mediated cell activation. In addition to the function as receptor for LPS, several other functions have been ascribed to CD14; next to the recognition of micro-organisms by the innate immune system CD14 also plays a role in cell-cell interactions.

Besides the membrane bound form of CD14, the soluble form of CD14 (sCD14), which lacks the GPI anchor, is also involved in LPS-induced cell activation. Two forms of sCD14 have been described. An approximately 48 kDa form, derived from monocytes membrane CD14, and a 56 kDa form, speculated to be directly released in plasma or supernatant after processing.

sCD14 affects LPS functioning via several pathways. sCD14 is an intermediate in the transfer of LPS to lipoproteins, resulting into neutralization of LPS. On the contrary, sCD14 facilitates LPS activation of CD14-membrane negative cells like endo- and epithelium. Furthermore, high concentrations of sCD14 were shown to block LPS-induced activation of monocytes. sCD14 thus both enhances and reduces cellular responses to LPS.

sCD14 was demonstrated to be present in plasma in levels ranging from 2 - 4 µg/ml and to be enhanced in infectious diseases.


## 3. KIT FEATURES

- Working time of 3½ hours.
- Minimum concentration which can be measured is 1.56 ng/ml.
- Measurable concentration range of 1.56 to 100 ng/ml.
- Working volume of 100 µl/well.

### Cross-reactivity

Cross-reactivity for other species or proteins/peptides has not been tested.

## 4. TEST PRINCIPLE

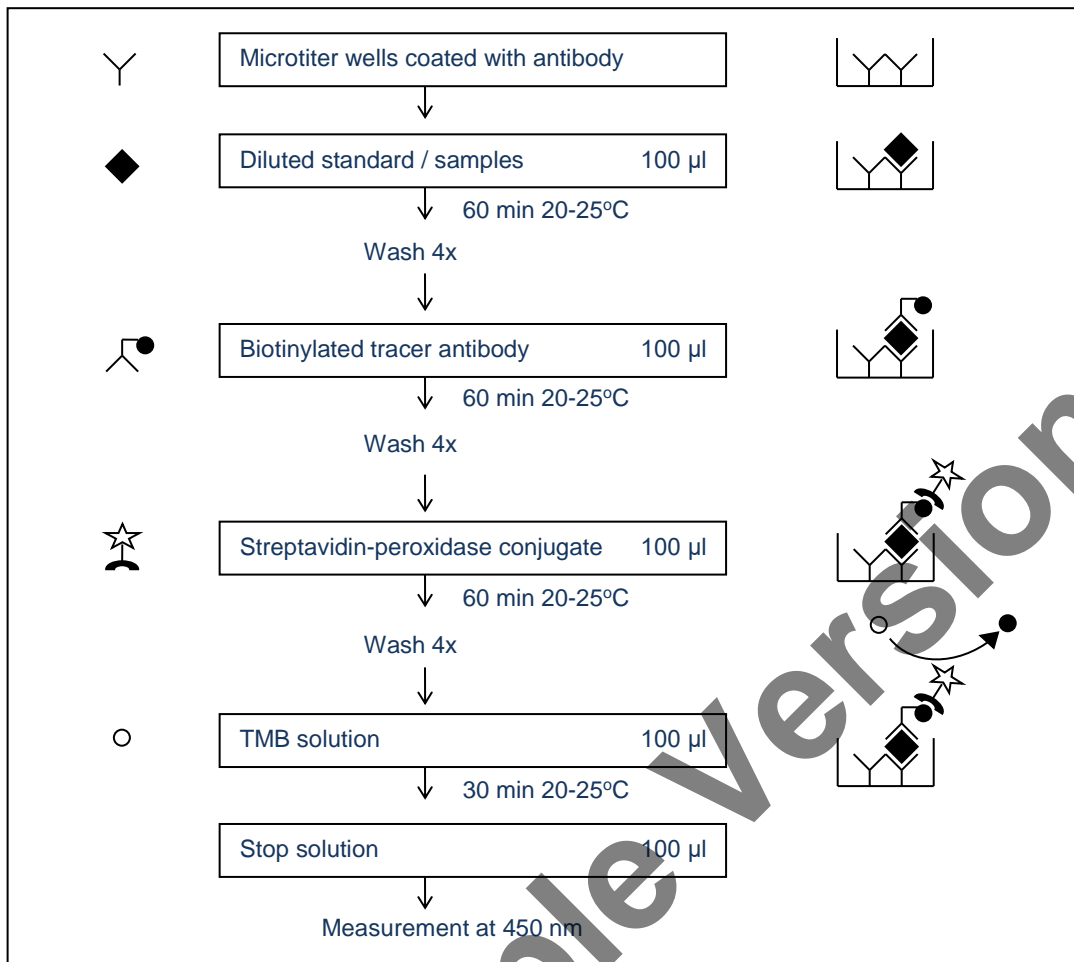

- The human sCD14 ELISA is a ready-to-use solid-phase enzyme-linked immunosorbent assay based on the sandwich principle with a working time of 3½ hours.
- The efficient format of a plate with twelve disposable 8-well strips allows free choice of batch size for the assay.
- Samples and standards are incubated in microtiter wells coated with antibodies recognizing human sCD14.
- Biotinylated tracer antibody will bind to captured human sCD14.
- Streptavidin-peroxidase conjugate will bind to the biotinylated tracer antibody.
- Streptavidin-peroxidase conjugate will react with the substrate, tetramethylbenzidine (TMB).
- The enzyme reaction is stopped by the addition of oxalic acid.
- The absorbance at 450 nm is measured with a spectrophotometer. A standard curve is obtained by plotting the absorbance (linear) versus the corresponding concentrations of the human sCD14 standards (log).
- The human sCD14 concentration of samples, which are run concurrently with the standards, can be determined from the standard curve.

## 5. TECHNICAL HINTS

- User should be trained and familiar with ELISA assays and test procedure.
- If you are not familiar with the ELISA technique it is recommended to perform a pilot assay prior to evaluation of your samples. Perform the assay with a standard curve only following the instructions.
- Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Completely empty wells before dispensing wash buffer, fill with wash buffer as indicated for each cycle and do not allow wells to sit uncovered or dry for extended periods.
- Since exact conditions may vary from assay to assay, a standard curve must be established for every run. Samples should be referred to the standard curve on the same plate.
- Do not mix reagents from different batches, or other reagents and strips. Remainers should not be mixed with contents of freshly opened vials.
- Each time the kit is used, fresh dilutions of standard, sample, tracer, streptavidin-peroxidase and buffers should be made.
- Caps and vials are not interchangeable. Caps should be replaced on the corresponding vials.
- To avoid cross-contaminations, change pipette tips between reagent additions of each standard, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.
- The waste disposal should be performed according to your laboratory regulations.

Example Version

## 6. REAGENT SUPPLIED

Kit component	Quantity RHK320-01R	Quantity RHK320-02R	Color code
Wash buffer 40x	1 vial (30 ml)	1 vial (30 ml)	Colorless
Dilution buffer 10x	1 vial (15 ml)	1 vial (15 ml)	Green
Standard	2 vials, lyophilized	4 vials, lyophilized	White
Tracer, biotinylated	1 vials, 1 ml lyophilized	2 vials, 1 ml lyophilized	White
Streptavidin-peroxidase 100x	1 tube, 0.25 ml in solution	1 tube, 0.25 ml in solution	Brown
TMB substrate	1 vial (11 ml)	1 vial (22 ml)	Brown
Stop solution	1 vial (22 ml)	1 vial (22 ml)	Red
12 Microtiter strips, pre-coated	1 plate	2 plates	

Table 1

- Upon receipt, store individual components at 2 - 8°C. Do not freeze.
- Do not use components beyond the expiration date printed on the kit label.
- The standard and tracer in lyophilized form and the streptavidin-peroxidase in concentrated solution are stable until the expiration date indicated on the kit label, if stored at 2 - 8°C.
- The exact amount of the standard is indicated on the label of the vial and the Certificate of Analysis.
- After reconstitution the standard is ready to use and cannot be stored.
- Once reconstituted the tracer is stable for 1 month if stored at 2 - 8°C.
- The streptavidin-peroxidase can only be stored in concentrated solution and is not stable when stored diluted.
- Upon receipt, foil pouch around the plate should be vacuum-sealed and unpunctured. Any irregularities to aforementioned conditions may influence plate performance in the assay.
- Return unused strips immediately to the foil pouch containing the desiccant pack and reseal along the entire edge of the zip-seal. Quality guaranteed for 1 month if stored at 2 - 8°C.

## 7. MATERIALS REQUIRED BUT NOT PROVIDED

- Calibrated micropipettes and disposable tips.
- Distilled or de-ionized water.
- Plate washer: automatic or manual.
- Polypropylene tubes.
- Calibrated ELISA plate reader capable of measuring absorbance at 450 nm.
- Adhesive covers can be ordered separately. Please contact your local distributor.

## 8. WARNINGS AND PRECAUTIONS

- For research use only, not for diagnostic or therapeutic use.
- This kit should only be used by qualified laboratory staff.
- Do not under any circumstances add sodium azide as preservative to any of the components.
- Do not use kit components beyond the expiration date.
- Do not mix reagents from different kits and lots. The reagents have been standardized as a unit for a given lot. Use only the reagents supplied by manufacturer.
- The assay has been optimized for the indicated standard range. Do not change the standard range.
- Open vials carefully: vials are under vacuum.
- Do not ingest any of the kit components.
- Kit reagents contain 2-chloroacetamide as a preservative. 2-Chloroacetamide is harmful in contact with skin and toxic if swallowed. In case of accident or if you feel unwell, seek medical advice immediately.
- The TMB substrate is light sensitive, keep away from bright light. The solution should be colorless until use.
- The stop solution contains 2% oxalic acid and can cause irritation or burns to respiratory system, skin and eyes. Direct contact with skin and eyes should be strictly avoided. If contact occurs, rinse immediately with plenty of water and seek medical advice.
- Incubation times, incubation temperature and pipetting volumes other than those specified may give erroneous results.
- Do not reuse microwells or pour reagents back into their bottles once dispensed.
- Handle all biological samples as potentially hazardous and capable of transmitting diseases.
- Hemolyzed, hyperlipemic, heat-treated or contaminated samples may give erroneous results.
- Use polypropylene tubes for preparation of standard and samples. Do not use polystyrene tubes or sample plates.

## 9. PREPARATION OF REAGENTS

Allow all the reagents to equilibrate to room temperature (20 – 25°C) prior to use. Return to proper storage conditions immediately after use.

### Wash buffer

Prepare wash buffer by mixing 30 ml of 40x wash buffer with 1170 ml of distilled or de-ionized water, which is sufficient for 2 x 96 tests. In case less volume is required, prepare the desired volume of wash buffer by diluting 1 part of the 40x wash buffer with 39 parts of distilled or de-ionized water.

### Dilution buffer

Prepare dilution buffer by mixing 15 ml of the 10x dilution buffer with 135 ml of distilled or de-ionized water, which is sufficient for 2 x 96 tests. In case less volume is required, prepare the desired volume of dilution buffer by diluting 1 part of the 10x dilution buffer with 9 parts of distilled or de-ionized water. Concentrated dilution buffer may contain crystals. In case the crystals do not disappear at room temperature within 1 hour, concentrated dilution buffer can be warmed up to 37°C. Do not shake the solution.

### Standard solution

The standard is reconstituted by pipetting the amount of dilution buffer mentioned on the CoA in the standard vial. Use the standard vial as Tube 1 in Figure 1. Prepare each human sCD14 standard in polypropylene tubes by serial dilution of the reconstituted standard with dilution buffer as shown in Figure 1\*. After reconstitution the standard cannot be stored for repeated use.

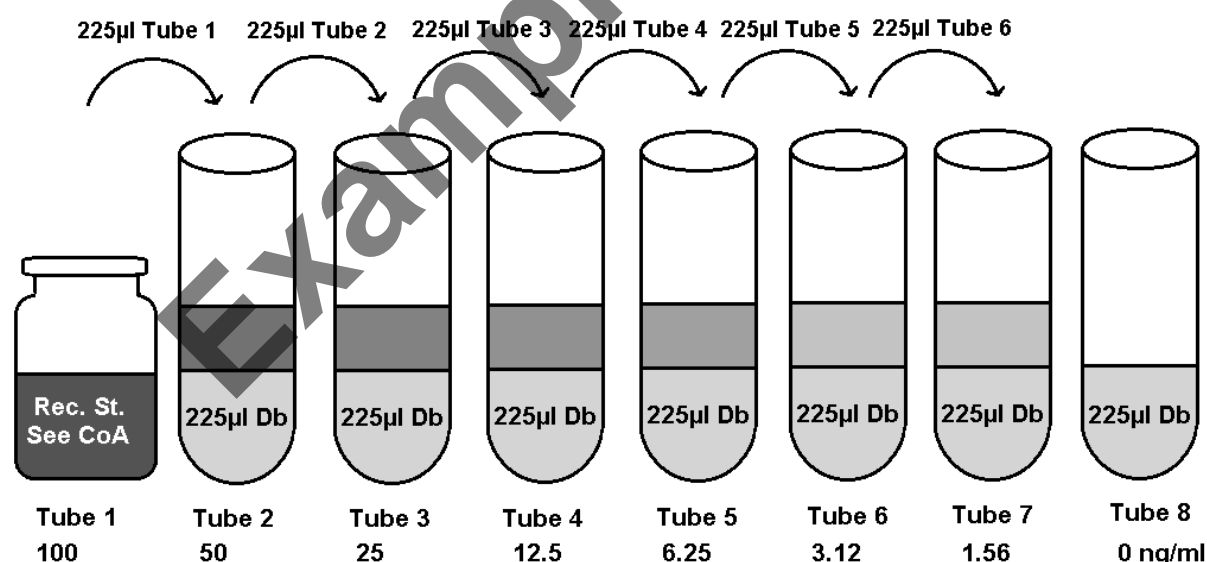


Figure 1

\*) CoA: Certificate of Analysis, Rec. St: Reconstituted Standard, Db: Dilution buffer

### Tracer solution

The tracer is reconstituted by pipetting 1 ml distilled or de-ionized water. Dilute the reconstituted 1 ml tracer with 11 ml dilution buffer, which is sufficient for 1 x 96 tests. In case less volume is required, prepare the desired volume of tracer by diluting 1 part of the reconstituted tracer with 11 parts of dilution buffer.



## Streptavidin-peroxidase solution

Prepare the streptavidin-peroxidase solution by mixing 0.25 ml of the 100x streptavidin-peroxidase solution with 24.75 ml dilution buffer, which is sufficient for 2 x 96 tests. In case less volume is required, prepare the desired volume of streptavidin-peroxidase solution by diluting 1 part of the 100x streptavidin-peroxidase solution with 99 parts of dilution buffer.

## 10. PREPARATION OF SAMPLES

### Collection and handling

#### Serum or plasma

Collect blood using normal aseptic techniques. Blood samples should be kept on ice. If serum is used, separate serum from blood after clotting at room temperature within 1 hour by centrifugation (1500xg at 4°C for 15 min). Transfer the serum to a fresh polypropylene tube.

If plasma is used, separate plasma from blood within 20 minutes after blood sampling by centrifugation (1500xg at 4°C for 15 min). Transfer the plasma to a fresh polypropylene tube.

Most reliable results are obtained if EDTA plasma is used.

#### Urine

Collect urine using normal aseptic techniques. Centrifuge the urine to remove debris (1500xg at 4 °C for 15 min). Transfer urine to a fresh polypropylene tube.

#### Storage

Store samples below -20°C, preferably at -70°C in polypropylene tubes. Storage at -20°C can affect recovery of human sCD14. Use samples within 24 hours after thawing. Avoid multiple freeze-thaw cycles which may cause loss of human sCD14 activity and give erroneous results.

Do not use hemolyzed, hyperlipemic, heat-treated or contaminated samples.

Before performing the assay, samples should be brought to room temperature (18 – 25°C) and mixed gently. Prepare all samples (controls and test samples) prior to starting the assay procedure. Avoid foaming.

### Dilution procedures

#### Serum or plasma samples

Human sCD14 can be measured accurately if serum or plasma samples are diluted at least 80x with supplied dilution buffer in polypropylene tubes.

Note that most reliable results are obtained with EDTA plasma.

#### Remark regarding recommended sample dilution

The mentioned dilution for samples is a minimum dilution and should be used as a guideline. The recovery of human sCD14 from an undiluted sample is not 100% and may vary from sample to sample. When testing less diluted samples it is advisable to run recovery experiments to determine the influence of the matrix on the detection of human sCD14.

Do not use polystyrene tubes or sample plates for preparation or dilution of the samples.

## 11. ASSAY PROCEDURE

Bring all reagents to room temperature (20 - 25°C) before use.

1. Determine the number of test wells required, put the necessary microwell strips into the supplied frame, and fill out the data collection sheet. Return the unused strips to the storage bag with desiccant, seal and store at 2 - 8°C.
2. Transfer 100 µl in duplicate of standard, samples, or controls into appropriate wells. Do not touch the side or bottom of the wells.
3. Cover the tray and tap the tray to eliminate any air bubbles. Be careful not to splash liquid onto the cover.
4. Incubate the strips or plate for 1 hour at room temperature.
5. Wash the plates 4 times with wash buffer using a plate washer or as follows\*:
  - a. Carefully remove the cover, avoid splashing.
  - b. Empty the plate by inverting plate and shaking contents out over the sink, keep inverted and tap dry on a thick layer of tissues.
  - c. Add 200 µl of wash buffer to each well, wait 20 seconds, empty the plate as described in 5b.
  - d. Repeat the washing procedure 5b/5c three times.
  - e. Empty the plate and gently tap on thick layer of tissues.
6. Add 100 µl of diluted tracer to each well using the same pipetting order as applied in step 2. Do not touch the side or bottom of the wells.
7. Cover the tray and incubate the tray for 1 hour at room temperature.
8. Repeat the wash procedure described in step 5.
9. Add 100 µl of diluted streptavidin-peroxidase to each well, using the same pipetting order as applied in step 2. Do not touch the side or bottom of the wells.
10. Cover the tray and incubate the tray for 1 hour at room temperature.
11. Repeat the wash procedure described in step 5.
12. Add 100 µl of TMB substrate to each well, using the same pipetting order as applied in step 2. Do not touch the side or bottom of the wells.
13. Cover the tray and incubate the tray for 30 minutes at room temperature. Avoid exposing the microwell strips to direct sunlight. Covering the plate with aluminium foil is recommended.
14. Stop the reaction by adding 100 µl of stop solution with the same sequence and timing as used in step 12. Mix solutions in the wells thoroughly by gently swirling the plate. Gently tap the tray to eliminate any air bubbles trapped in the wells.
15. Read the plate within 30 minutes after addition of stop solution at 450 nm using a plate reader, following the instructions provided by the instrument's manufacturer.

\*) In case plate washer is used, please note: use of a plate washer can result in higher background and decrease in sensitivity. We advise validation of the plate washer with the manual procedure.

Make sure the plate washer is used as specified for the manual method.

## 12. CALCULATIONS

- Calculate the mean absorbance for each set of duplicate standards, control and samples.
- If individual absorbance values differ by more than 15% from the corresponding mean value, the result is considered suspect and the sample should be retested.
- The mean absorbance of the zero standard should be less than 0.3.
- Create a standard curve using computer software capable of generating a good curve fit. The mean absorbance for each standard concentration is plotted on the vertical (Y) axis versus the corresponding concentration on the horizontal (X) axis (logarithmic scale).
- If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.
- Samples that give a mean absorbance above the absorbance for the highest standard concentration are out of range of the assay. These samples should be retested at a higher dilution

## 13. QUALITY CONTROL

The Certificate of Analysis is lot specific and is to be used to verify results obtained by your laboratory. The absorption values provided on the Certificate of Analysis are to be used as a guideline only. The results obtained by your laboratory may differ.

This assay is designed to eliminate interference by soluble receptors, binding proteins, and other factors present in biological samples. Until all factors have been tested in the BioVendor immunoassay, the possibility of interference cannot be excluded.

For optimal performance of this kit, it is advised to work according to good laboratory practice.

## 14. TROUBLESHOOTING

Warranty claims and complaints in respect of deficiencies must be logged before expiry date of the product. A written complaint containing lot number of the product and experimental data should be sent to [info@biovendor.com](mailto:info@biovendor.com).

Suggestions summarized below in Table 2 can be used as a guideline in the case of unexpected assay results.

Low absorbance	High absorbance	Poor duplicates	All wells positive	All wells negative	Possible cause
•	•		•	•	Kit materials or reagents are contaminated or expired
•					Incorrect reagents used
•		•	•		Lyophilized reagents are not properly reconstituted
•	•	•	•	•	Incorrect dilutions or pipetting errors
•		•			Improper plastics used for preparation of standard and/or samples
•	•				Improper incubation times or temperature
		•			Especially in case of 37°C incubation: plates are not incubated uniformly
•					Assay performed before reagents were brought to room temperature
•	•	•	•	•	Procedure not followed correctly
				•	Omission of a reagent or a step
		•			Poor mixing of samples
	•		•		Low purity of water
	•	•			Strips were kept dry for too long during/after washing
	•	•	•		Inefficient washing
	•	•			Cross-contamination from other samples or positive control
		•	•		TMB solution is not clear or colorless
•	•				Wrong filter in the microtiter reader










Low absorbance	High absorbance	Poor duplicates	All wells positive	All wells negative	Possible cause
	•	•			Airbubbles
		•			Imprecise sealing of the plate after use
•					Wrong storage conditions
•					Lamp in microplate reader is not functioning optimally

Table 2

## 15. REFERENCES

1. Dentener, M et al; Bacterial/permeability-increasing protein release in whole blood ex vivo: strong induction by lipopolysaccharide and tumor necrosis factor-alpha. J Infect Dis 1996, 175: 108
2. Hiltermann, J et al; Ozone-induced inflammation assessed in sputum and bronchial lavage fluid from asthmatics: a new noninvasive tool in epidemiologic studies on air pollution and asthma. Free Radic Biol Med 1999, 27: 1448
3. Blais, D et al; Killing the messenger in the nick of time: persistence of breast milk sCD14 in the neonatal gastrointestinal tract. Pediatr Res 2006, 59: 371
4. Poikonen, K et al; Susceptibility of human monocyte-macrophages to *Chlamydia pneumoniae* infection *in vitro* is highly variable and associated with levels of soluble CD14 and *C. pneumoniae* IgA and human HSP-IgG antibodies in serum. Scand J Immunol 2008, 67: 279

## 16. EXPLANATION OF SYMBOLS

	Catalogue number
	Batch code
	Caution
	Use by date
	Temperature limit
	Manufacturer
 <a href="http://www.biovendor.com">www.biovendor.com</a>	Read electronic instructions for use - eIFU
	The content is sufficient for 96 tests
	Biological risks



BioVendor – Laboratorní medicína a.s.  
Karásek 1767/1, 621 00 Brno, Czech Republic  
+420 549 124 185  
[info@biovendor.com](mailto:info@biovendor.com)  
[sales@biovendor.com](mailto:sales@biovendor.com)  
[www.biovendor.com](http://www.biovendor.com)

Example Version

