

BioVendor

Research
and Diagnostic Products



HUMAN ALPHA-FETOPROTEIN (AFP) ELISA

Product Data Sheet

Cat. No.: RIS0018R

For Research Use Only

CONTENTS

1.	INTENDED USE	3
2.	STORAGE, EXPIRATION	3
3.	INTRODUCTION	3
4.	TEST PRINCIPLE	4
5.	PRECAUTIONS	4
6.	TECHNICAL HINTS	5
7.	REAGENT SUPPLIED	5
8.	MATERIAL REQUIRED BUT NOT SUPPLIED	6
9.	PREPARATION OF REAGENTS	6
10.	PREPARATION OF SAMPLES	7
11.	ASSAY PROCEDURE	8
12.	CALCULATIONS	8
13.	PERFORMANCE CHARACTERISTICS	9
14.	QUALITY CONTROL	12
15.	LIMITATIONS	12
16.	LEGAL ASPECTS	13
17.	REFERENCES	14

**»» This kit is manufactured by:
BioVendor – Laboratorní medicína a.s.**

»» Use only the current version of Product Data Sheet enclosed with the kit!

1. INTENDED USE

The RIS0018R Human alpha-Fetoprotein (AFP) ELISA Immunoenzymetric assay for the research use only of alpha-fetoprotein (AFP) in serum.

This kit is not intended to be used for the risk evaluation of trisomy 21.. It is intended for research use only.

2. STORAGE, EXPIRATION

When stored at 2-8°C unopened reagents will retain reactivity until expiration date. Do not use reagents beyond this date.

Opened reagents must be stored at 2-8°C. Microtiter wells must be stored at 2-8°C. Once the foil bag has been opened, care should be taken to close it tightly again.

Opened kits retain activity for six weeks if stored as described above.

3. INTRODUCTION

Alpha-Fetoprotein (AFP) is a glycoprotein with a molecular weight of approximately 70 KD(1). AFP is normally produced during fetal and neonatal development by the liver, yolk sac, and in small concentrations by the gastrointestinal tract (2). After birth, serum AFP concentrations decrease rapidly, and by the second year of life and thereafter only trace amounts are normally detected in serum (3).

Elevation of serum AFP to abnormally high values occurs in several malignant diseases (4-7), most notably nonseminomatous testicular cancer and primary hepatocellular carcinoma. In the case of nonseminomatous testicular cancer, a direct relationship has been observed between the incidence of elevated AFP levels and the stage of disease (8-9). Elevated AFP levels have also been observed in patients diagnosed with seminoma with nonseminomatous elements, but not in patients with pure seminoma (6,8,10-11).

In addition, elevated serum AFP concentrations have been measured in patients with other noncancerous diseases, including ataxia telangiectasia, hereditary tyrosinemia, neonatal hyperbilirubinemia, acute viral hepatitis, chronic active hepatitis and cirrhosis (12-15). Elevated serum AFP concentrations are also observed in pregnant women (16-17). Therefore, AFP measurements are not recommended for use as a screening procedure to detect the presence of cancer in the general population.

4. TEST PRINCIPLE

The Biovendor AFP ELISA Kit is a solid phase enzyme-linked immunosorbent assay (ELISA) based on the sandwich principle.

The microtiter wells are coated with a monoclonal [mouse] antibody directed towards a unique antigenic site on an AFP molecule. An aliquot of patient sample containing endogenous AFP is incubated in the coated well with enzyme conjugate, which is an anti- AFP antibody conjugated with horseradish peroxidase. After incubation the unbound conjugate is washed off. The amount of bound peroxidase is proportional to the concentration of AFP in the sample.

Having added the substrate solution, the intensity of colour developed is proportional to the concentration of AFP in the patient sample.

5. PRECAUTIONS

Safety

For research use only

For information on hazardous substances included in the kit please refer to Material Safety Data Sheets.

All reagents of this test kit which contain human serum or plasma have been tested and confirmed negative for HIV I/II, HBsAg and HCV by FDA approved procedures. All reagents, however, should be treated as potential biohazards in use and for disposal.

Avoid contact with *Stop Solution* containing 0.5 M H₂SO₄. It may cause skin irritation and burns.

Never pipet by mouth and avoid contact of reagents and specimens with skin and mucous membranes.

Do not smoke, eat, drink or apply cosmetics in areas where specimens or kit reagents are handled.

Wear disposable latex gloves when handling specimens and reagents. Microbial contamination of reagents or specimens may give false results.

Handling should be in accordance with the procedures defined by an appropriate national biohazard safety guideline or regulation.

Do not use reagents beyond expiry date as shown on the kit labels.

All indicated volumes have to be performed according to the protocol. Optimal test results are only obtained when using calibrated pipettes and microtiterplate readers.

Do not mix or use components from kits with different lot numbers. It is advised not to exchange wells of different plates even of the same lot. The kits may have been shipped or stored under different conditions and the binding characteristics of the plates may result slightly different.

Chemicals and prepared or used reagents have to be treated as hazardous waste according the national biohazard safety guideline or regulation.

6. TECHNICAL HINTS

All reagents and specimens must be allowed to come to room temperature before use. All reagents must be mixed without foaming.

Once the test has been started, all steps should be completed without interruption.

Use new disposal plastic pipette tips for each calibrator, control or sample in order to avoid cross contamination

Absorbance is a function of the incubation time and temperature. Before starting the assay, it is recommended that all reagents are ready, caps removed, all needed wells secured in holder, etc. This will ensure equal elapsed time for each pipetting step without interruption.

As a general rule the enzymatic reaction is linearly proportional to time and temperature.

7. REAGENT SUPPLIED



12x8 (break apart) strips, 96 wells;
Wells coated with anti-AFP antibody (monoclonal).

CAL	N
-----	---

N=1 to 4, 4 vials (lyophilized), 0.5 mL;

See exact values on the vial label

Conversion: 1IU/mL = 1,21ng/mL

The calibrators are calibrated against NIBSC 1st International Standard for Alphafoetoprotein AFP (AFP 1st IRP 72/225)

See „Preparation of Reagents“;

* contain 0.03% Proclin 300, 0.015% BND and 0.010% MIT as a preservative.

CAL	0
-----	---

Zero Calibrator, 1 vial (lyophilized), 0.5 ml

* contain 0.03% Proclin 300, 0.015% BND and 0.010% MIT as a preservative.

See „Preparation of Reagents“

Ab	HRP
----	-----

(Enzyme conjugate) 1 vial, 11 mL, ready to use,

Anti-AFP antibody conjugated to horseradish peroxidase;

contains 0.03% Proclin 300 as a preservative.

CHROM	TMB
-------	-----

(Substrate solution) 1 vial, 14 mL, ready to use,
Tetramethylbenzidine (TMB).

STOP	STOLN
------	-------

(Stop solution) 1 vial, 14 mL, ready to use,
contains 0.5 M H₂SO₄.

Avoid contact with the stop solution. It may cause skin irritations and burns.

BND = 5-bromo-5-nitro-1,3-dioxane

MIT = 2-methyl-2H-isothiazol-3-one

Note: Additional Calibrator 0 for sample dilution is available on request.

8. MATERIAL REQUIRED BUT NOT SUPPLIED

A microtiter plate calibrated reader (450 ± 10 nm)
Calibrated variable precision micropipettes.
Absorbent paper.
Bidistilled water

9. PREPARATION OF REAGENTS

Allow all reagents and required number of strips to reach room temperature prior to use.

➤➤ Calibrators

Reconstitute the lyophilized contents of the calibrator vial with 0.5 mL bidistilled water!

Note: The reconstituted calibrators are stable for 2 months at 2-8°C. For longer storage freeze at -20°C.

➤➤ Disposal of the Kit

The disposal of the kit must be made according to the national regulations. Special information for this product is given in the Material Safety Data Sheets.

»» Damaged Test Kits

In case of any severe damage of the test kit or components, Biovendor have to be informed written, latest one week after receiving the kit. Severely damaged single components should not be used for a test run. They have to be stored until a final solution has been found. After this, they should be disposed according to the official regulations.

10. PREPARATION OF SAMPLES

Serum should be used in this assay.

Do not use haemolytic, icteric or lipaemic specimens.

NOTE: Samples containing sodium azide should not be used in the assay.

NOTE: If an amniocentesis is necessary the specimen collection has to be done before the puncture. After the amniotic puncture increased AFP values are determined.

- **Specimen Collection**

Serum:

Collect blood by venipuncture (e.g. Sarstedt Monovette # 02.1388.001), allow to clot, and separate serum by centrifugation at room temperature. Do not centrifuge before complete clotting has occurred. Patients receiving anticoagulant therapy may require increased clotting time.

- **Specimen Storage**

Specimens should be capped and may be stored for up to 5 days at 2-8°C prior to assaying. Specimens held for a longer time should be frozen only once at -20°C prior to assay. Thawed samples should be inverted several times prior to testing.

- **Specimen Dilution**

If in an initial assay, a specimen is found to contain more than the highest calibrator, the specimens can be diluted with *Calibrator 0* and reassayed as described in Assay Procedure.

For the calculation of the concentrations this dilution factor has to be taken into account.

Example:

a) dilution 1:10: 10 µL Serum + 90 µL *Calibrator 0* (mix thoroughly)

b) dilution 1:100: 10 µL dilution a) 1:10 + 90 µL *Calibrator 0* (mix thoroughly).

11. ASSAY PROCEDURE

Each run must include a calibration curve.

1. Secure the desired number of Microtiter wells in the frame holder.
2. Dispense **25 µL** of each **Calibrator, Control** and **samples** with new disposable tips into appropriate wells.
3. Dispense **100 µL Enzyme Conjugate** into each well.
Thoroughly mix for 10 seconds. It is important to have a complete mixing in this step.
4. Incubate for **30 minutes** at room temperature.
5. Briskly shake out the contents of the wells.
Rinse the wells 5 times with distilled water (400 µL per well). Strike the wells sharply on absorbent paper to remove residual droplets.
Important note:
The sensitivity and precision of this assay is markedly influenced by the correct performance of the washing procedure!
6. Add **100 µL of Substrate Solution** to each well.
7. Incubate for **10 minutes** at room temperature.
8. Stop the enzymatic reaction by adding **50 µL of Stop Solution** to each well.
Determine the absorbance (OD) of each well at **450±10 nm** with a microtiter plate reader.
It is recommended that the wells be read **within 10 minutes** after adding the *Stop Solution*.

12. CALCULATIONS

Calculate the average absorbance values for each set of calibrators, controls and patient samples.

Construct a calibration curve by plotting the mean absorbance obtained from each calibrator against its concentration with absorbance value on the vertical(Y) axis and concentration on the horizontal (X) axis.

Using the mean absorbance value for each sample determine the corresponding concentration from the calibration curve.

Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results.

The concentration of the samples can be read directly from this calibration curve. Samples with concentrations higher than that of the highest calibrator have to be further diluted. For the calculation of the concentrations this dilution factor has to be taken into account.

Example of Typical Calibration curve

The following data is for demonstration only and cannot be used in place of data generations at the time of assay.

Calibrator	Optical Units (450 nm)
Calibrator 0 (0 IU/mL)	0.07
Calibrator 1 (10 IU/mL)	0.21
Calibrator 2 (40 IU/mL)	0.69
Calibrator 3 (80 IU/mL)	1.29
Calibrator 4 (160 IU/mL)	1.97

13. PERFORMANCE CHARACTERISTICS

- **Assay Dynamic Range**

The range of the assay is between 1.78 – 160 IU/mL.

- **Specificity of Antibodies (Cross Reactivity)**

The following substances were tested for cross reactivity of the assay:

Protein	Produced Color Intensity Equivalent to AFP in serum (IU/mL)
HSA 20 mg/ml	2
Prolaktin 200 ng/ml	2
hCG 2000 ng/ml	2
SP- 1 2000 ng/ml	2
hPL 2011 µg/ml	2

- **Analytical Sensitivity**

The analytical sensitivity was calculated from the mean plus two standard deviations of twenty (20) replicate analyses of Calibrator 0 and was found to be 1.78 IU/mL.

- **Precision**

Intra Assay Variation (n=20)

The within assay variability is shown below:

Sample	Mean (IU/mL)	CV (%)
1	25.63	3.82
2	105.78	5.39

3	77.63	3.50
---	-------	------

Inter Assay Variation (n=16)

The inter assay variability (between run is shown below:

Sample	Mean (IU/mL)	CV (%)
1	25.31	3.64
2	109.34	6.54
3	84.10	6.74

- **Recovery**

Recovery of the Biovendor ELISA was determined by adding increasing amounts of the analyte to three sera of pregnant women. The percentage recoveries were determined by comparing expected and measured values of the samples.

		Sample 1	Sample 2	Sample 3
Concentration [IU/mL]		30.86	115.20	69.02
Average Recovery		92.9	94.0	99.1
Range of Recovery [%]	from	86.7	93.4	92.6
	to	99.5	94.7	106.5

- **Linearity**

Three samples (serum) containing different amounts of analyt were serially diluted (up to 1:16) with zero calibrator and assayed with the Biovendor ELISA. The percentage recovery was calculated by comparing the expected and measured values for the analyt.

		Sample 1	Sample 2	Sample 3
Concentration [IU/mL]		39.7	75.6	128.4
Average Recovery		102.0	95.5	96.8
Range of Recovery [%]	from	90.9	86.2	92.9
	to	115.0	109.3	101.3

- **Expected values**

It is strongly recommended that each laboratory should determine its own normal and abnormal values.

In a study conducted using the Biovendor AFP ELISA the following values are observed:

Normal healthy adults, non-pregnant

The lower limit of AFP concentration in normal serum is less than 1 IU/mL; the upper limit is about 10 IU/mL.

Values during pregnancy

Weeks of pregnancy	AFP [IU/mL]
10	9 - 24
11	10 - 27
12	10 - 30
13	10 - 34
14	11 - 45
15	14 - 60
16	16 - 69
17	17 - 78
18	22 - 93

Weeks of pregnancy	AFP [IU/mL]
19	32 - 103
20	42 - 121
21	48 - 139
22 - 24	56 - 224
25 - 27	95 - 357
28 - 30	135 - 435
31 - 33	141 - 423
34 - 36	121 - 380
37 - 40	93 - 321

- **Clinical importance**

Maternal serum containing AFP above 2.5 times the normal median for weeks 16 to 18 of pregnancy was detected in 88% of cases of anencephaly and in 79% of cases of open spina bifida.

The concentration of AFP in hepatocellular carcinoma and germ cell tumor varies from the normal range up to several million IU/ml. After surgical resection, the serum AFP may drop to normal range or somewhat above it.

AFP may occur in serum of patients with diseases other than hepatocarcinoma or embryonal carcinoma of the testes, such as neonatal hepatitis and nonhepatic neoplasms.

14. QUALITY CONTROL

- Good laboratory practice requires that controls be run with each calibration curve. A statistically significant number of controls should be assayed to establish mean values and acceptable ranges to assure proper performance.
- It is recommended to use control samples according to state and federal regulations. The use of control samples is advised to assure the day to day validity of results. Use controls at both normal and pathological levels.
- The controls and the corresponding results of the QC-Laboratory are stated in the QC certificate added to the kit. The values and ranges stated on the QC sheet always refer to the current kit lot and should be used for direct comparison of the results.
- It is also recommended to make use of national or international Quality Assessment programs in order to ensure the accuracy of the results.
- Employ appropriate statistical methods for analysing control values and trends. If the results of the assay do not fit to the established acceptable ranges of control materials patient results should be considered invalid.
- In this case, please check the following technical areas: Pipetting and timing devices; photometer, expiration dates of reagents, storage and incubation conditions, aspiration and washing methods.

15. LIMITATIONS

Interfering Substances

Any improper handling of samples or modification of this test might influence the results. Haemoglobin (up to 4 mg/mL), Bilirubin (up to 0.5 mg/mL) and Triglyceride (up to 30 mg/mL) have no influence on the assay results.

Drug Interferences

Until today no substances (drugs) are known to us, which have an influence to the measurement of AFP in a sample.

High-Dose-Hook Effect

No hook effect was observed in this test up to 1600 IU/mL of AFP.

16. LEGAL ASPECTS

Reliability of Results

The test must be performed exactly as per the manufacturer's instructions for use. Moreover the user must strictly adhere to the rules of GLP (Good Laboratory Practice) or other applicable national standards and/or laws. This is especially relevant for the use of control reagents. It is important to always include, within the test procedure, a sufficient number of controls for validating the accuracy and precision of the test.

The test results are valid only if all controls are within the specified ranges and if all other test parameters are also within the given assay specifications. In case of any doubt or concern please contact Biovendo.

Therapeutic Consequences

Therapeutic consequences should never be based on laboratory results alone even if all test results are in agreement with the items as stated under point 11.1. Any laboratory result is only a part of the total clinical picture of a patient.

Only in cases where the laboratory results are in acceptable agreement with the overall clinical picture of the patient should therapeutic consequences be derived.

The test result itself should never be the sole determinant for deriving any therapeutic consequences.

Liability

Any modification of the test kit and/or exchange or mixture of any components of different lots from one test kit to another could negatively affect the intended results and validity of the overall test. Such modification and/or exchanges invalidate any claim for replacement.

Claims submitted due to customer misinterpretation of laboratory results subject to point 11.2. are also invalid. Regardless, in the event of any claim, the manufacturer's liability is not to exceed the value of the test kit. Any damage caused to the test kit during transportation is not subject to the liability of the manufacturer.


17. REFERENCES

»» References to alpha-fetoprotein (AFP):

1. Ruoslahti, E. and Seppala, M., Studies of Carcino-Fetal Proteins: Physical and Chemical Properties of Human Alpha-Fetoprotein. *Int. J. Cancer* 7:218, 1971.
2. Gitlin, D., Perricelli, A. and Gitlin, G. M., Synthesis of Alpha-Fetoprotein by Liver, Yolk Sac, and Gastrointestinal Tract of the Human Conceptus. *Cancer Res.* 32:979, 1972.
3. Masseyeff, R., Gilli, G., Krebs, B., Bonet, C. and Zrihen, H., Evolution en Fonction de l'Age du Taux Serique Physiologique de l'Alpha-Foetoproteine chez l'Homme et le Rat. (French) in *Alpha-Feto-Protein* (Masseyeff, R., ed.) p.313. INSERM, Paris, 1974.
4. Silver, H. K. B., Gold, P., Feder, S., Freedman, So. O. and Shuster, J., Radioimmunoassay for human alpha-fetoprotein. *Proc. Nat. Acad. Sci. U.S.A.* 70:526, 1973.
5. Waldmann, T. A. and McIntire, K. R., The use of a radioimmunoassay for alpha-fetoprotein in the diagnosis of malignancy. *Cancer* 34:1510, 1974.
6. Kohn, J., Orr, A.H. McElwain, T.J., Bentall, M. and Peckham, M. J., Serum alpha-fetoprotein in patients with testicular tumors. *Lancet* 2:433, 1976.
7. Abelev, G.I., Alpha-fetoprotein in ontogenesis and its association with malignant tumors. *Adv. Cancer Res.* 14: 295, 1971.
8. Scardino, P. T., Cox, H. D., Waldermann, T. A., McIntire, K. R., Mitemeyer, B. and Javadpour, N., The value of the serum tumor markers in the staging and prognosis of germ cell tumors of the testis. *J. Urol.* 118:994, 1977.
9. Bosl, G.J., Lange, P. H., Fraley, E. E., Goldman, A., Nochomovitz, L. E., Rosai, J., et al., Human chorionic gonadotropin and alpha-fetoprotein in the staging of nonseminomatous testicular cancer. *Cancer* 47:328, 1981
10. Lange, P.H., McIntire, K.R. and Waldmann, T. A., Hakala, T.R. and Fraley, E. E., Serum alpha-fetoprotein and human chorionic gonadotropin in the diagnosis and management of nonseminomatous germ-cell testicular cancer. *Medical Intelligence* 259:1237, 1976.
11. Javadpour, N., McIntire, K. R. and Waldmann, T. A., Human chorionic gonadotropin (HCG) and alpha-fetoprotein (AFP) in sera and tumor cells of patients with testicular seminoma. *Cancer* 42:2768, 1978.
12. Waldmann, T.A. and McIntire, K. R., Serum Alpha-Fetoprotein Levels in Patients with Ataxia-Telangiectasia. *Lancet* 2:1112, 1972.
13. Belanger, L., Tyrosinémie Héritaire et Alpha-1-Fetoprotéine. II. Recherche Tissulaire Comparée de l'Alpha-Foetoprotéine dans Deux Cas de Tyrosinémie Héritaire. Considérations sur l'Ontogenèse de la Foetoprotéine Humaine (French). *Pathol. Bio.*21:457, 1973.
14. Kew, M. C., Purves, L.R. and Bersohn, I., Serum Alpha-Fetoprotein Levels in Acute Viral Hepatitis. *Gut* 14:939, 1973.
15. Endo, Y., Kanai, K., Oda, T., Mitamura, K., Iino, S. and Suzuki, H., Clinical Significance of alpha-Fetoprotein in Hepatitis and Liver Cirrhosis. *Ann. N. Y. Acad. Sci.* 259:234, 1975.
16. Purves, L. R. and Purves M., Serum Alpha-Fetoprotein. VI. The Radioimmunoassay Evidence for the Presence of AFP in the Serum of Normal People and During Pregnancy. *S. Afr. Med. J.* 46:1290, 1972.

17. Sepalla, M. and Ruoslahti, E., Alpha-Fetoprotein: Physiology and Pathology During Pregnancy and Application to Antenatal Diagnosis. *J. Perinat. Med.* 1:104, 1973.
18. Engvall, E., *Methods in Enzymology*, Volume 70, Van Vunakis, H. and Langone, J.J. (eds.) Academic Press, New York, NY, 419 (1980).
19. Uotila, M., Ruoslahti, E. and Engvall, E., *J. Immunol. Methods*, 42, 11 (1981).

➤➤ For more references on this product see our WebPages at www.biovendor.com

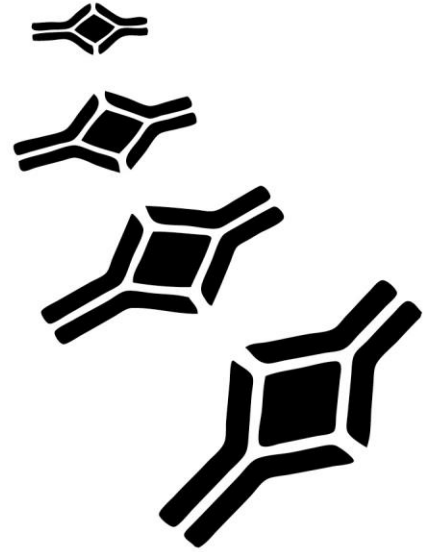

BioVendor – Laboratorní medicína a.s.

Karasek 1767/1, 621 00 Brno, Czech Republic

Phone: +420-549-124-185, Fax: +420-549-211-460

E-mail: info@biovendor.com, sales@biovendor.com

Web: www.biovendor.com

There are BioVendor branches and distributors near you.

To find the office closest to you, visit www.biovendor.com/contact

